


1EN2FR3DE4IT5ES6NL7RU8TR9AR

OMRON

Automatic Upper Arm Blood Pressure Monitor

M3 Comfort (HEM-7134-E) Instruction Manual



IM-HEM-7134-E-EN-03-04/2018  
3270152-8C

Introduction

Thank you for purchasing the OMRON M3 Comfort Automatic Upper Arm Blood Pressure Monitor.

The OMRON M3 Comfort is a compact, fully automatic upper arm blood pressure monitor, operating on the oscillometric principle. It measures your blood pressure and pulse rate simply and quickly. For comfortable controlled inflation without the need of pressure pre-setting or re-inflation the device uses its advanced "IntelliSense" technology.

**Intended Use**  
This device is a digital monitor intended for use in measuring blood pressure and pulse rate in adult patient population who can understand this instruction manual with the arm circumference range printed on the arm cuff. The device detects the appearance of irregular heartbeats during measurement and gives a warning signal with the measurement result. It is mainly designed for general household use.

Please follow this instruction manual thoroughly for your safety.  
Please keep for future reference. For specific information about your own blood pressure, CONSULT YOUR PHYSICIAN.

Important Safety Information

**Warning: Indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.**

- (General Usage)**
- DO NOT adjust medication based on measurement results from this blood pressure monitor. Take medication as prescribed by your physician. Only a physician is qualified to diagnose and treat High Blood Pressure.
  - Consult your physician before using the device for any of the following conditions: common arrhythmias such as atrial or ventricular premature beats or atrial fibrillation, arterial sclerosis, poor perfusion, diabetes, age, pregnancy, pre-eclampsia, renal diseases. Note that PATIENT motion, trembling, shivering may affect the measurement reading.
  - Do not use the device on the injured arm or the arm under medical treatment.
  - Stop using the device and consult your physician if you experience skin irritation or other troubles.
  - Do not apply the arm cuff on the arm while being on an intravenous drip or blood transfusion.
  - Consult your physician before using the device on the arm with an arterio-venous (A-V) shunt.
  - Do not use the device with other medical electrical (ME) equipment simultaneously. This may result in an incorrect operation of the device and/or cause an inaccurate reading.
  - Do not use the device in the area the HF surgical equipment, MRI, or CT scanner exists, or in the oxygen rich environment. This may result in an incorrect operation of the device and/or cause an inaccurate reading.
  - The air tube or the AC adapter cable may cause accidental strangulation in infants.
  - Contained small parts that may cause a choking hazard if swallowed by infants.
- (AC Adapter (optional) Usage)**
- Do not use the AC adapter if the device or the power cord is damaged. Turn off the power and unplug the power cord immediately.
  - Plug the AC adapter into the appropriate voltage outlet. Do not use in a multi-outlet plug.
  - Never plug in or unplug the power cord from the electric outlet with wet hands.

**Caution: Indicates a potentially hazardous situation which, if not avoided, may result in minor or moderate injury to the user or patient or damage to the equipment or other property.**

- (General Usage)**
- Always consult your physician. Self-diagnosis of measurement results and self-treatment are dangerous.
  - People with severe blood flow problems, or blood disorders, should consult a physician before using the device, as the arm cuff inflation can cause bruising.
  - Remove the arm cuff if it does not start deflating during the measurement.
  - Do not use this device on infants or persons who cannot express their intentions.
  - Do not use the device for any purpose other than measuring blood pressure.
  - Use only the approved arm cuff for this device. Use of other arm cuffs may result in incorrect measurement results.
  - During measurement, make sure that no mobile phone or any other electrical devices that emit electromagnetic fields is within 30cm of this device. This may result in incorrect operation of the device and/or cause an inaccurate reading.
  - Do not disassemble the monitor or arm cuff. This may cause an inaccurate reading.
  - Do not use in a location with moisture, or a location where water may splash on the device. This may damage the device.
  - Do not use the device in a moving vehicle (car, airplane).
  - Do not take measurements more than necessary. It may cause bruising due to blood flow interference.
  - Consult your physician before using the device if you had a mastectomy.
  - Read "If your systolic pressure is more than 210 mmHg" of this instruction manual, if your systolic pressure is known to be more than 210 mmHg. Inflating to a higher pressure than necessary may result in bruising where the cuff is applied.

- (AC Adapter (optional) Usage)**
- Fully insert the power plug into the outlet.
  - When disconnecting the power plug from the outlet, do not pull the power cord. Be sure to pull from the power plug safely.
  - When handling the power cord, take care not to do the following:
    - Do not damage. Do not break it.
    - Do not tamper with it. Do not forcibly bend or pull.
    - Do not twist. Do not bundle during use.
    - Do not pinch. Do not place under heavy objects.

- Wipe the dust off from the power plug.
- Unplug monitor when not in use.
- Disconnect the power plug before cleaning.
- Use only an OMRON AC adapter designed for this device. Use of unsupported adapters may damage and/or may be hazardous to the device.

- (Battery Usage)**
- Do not insert the batteries with their polarities incorrectly aligned.
  - Use only 4 "AA" alkaline or manganese batteries with this device. Do not use other types of batteries. Do not use new and used batteries together.
  - Remove the batteries if the device will not be used for three months or more.
  - Use the battery within recommended period mentioned to it.


- General Precautions**
- Do not forcibly crease the arm cuff or the air tube excessively.
  - Do not fold or kink the air tube while taking a measurement. This may cause harmful injury by interrupting blood flow.

- To unplug the air plug, pull on the air plug at the connection with the monitor, not the tube itself.
- Do not drop the monitor or subject device to strong shocks or vibrations.
- Do not inflate the arm cuff when it is not wrapped around your arm.
- Do not use the device outside the specified environment. It may cause an inaccurate reading.
- Read and follow the "Important information regarding Electro Magnetic Compatibility (EMC)" in the "6. Specifications".
- Read and follow the "Correct Disposal of This Product" in "6. Specifications" when disposing of the device and any used accessories or optional parts.
- Please check (for example, by observation of the limb concerned) if the device is not causing a prolonged impairment of PATIENT blood circulation.
- If the device is stored at the maximum or minimum storage and transport temperature and is moved to an environment with a temperature of 20°C, we recommend waiting for approximately 2 hours before using the device.


1. Know Your Device

**Contents:**  
Monitor, arm cuff, instruction manual, storage case, battery set, blood pressure diary


Monitor:

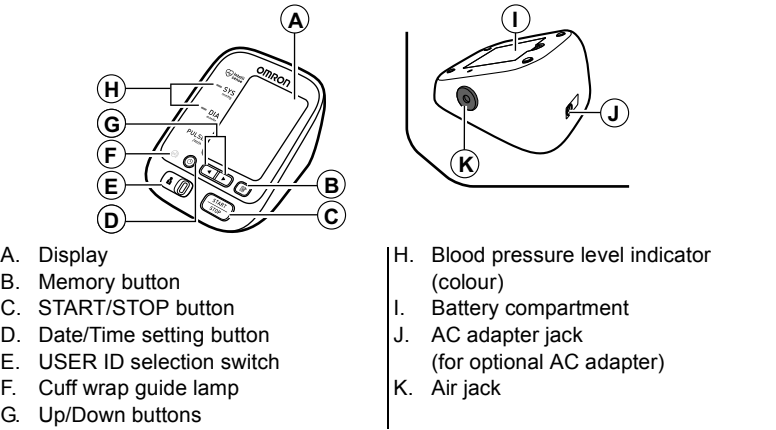

Arm cuff:

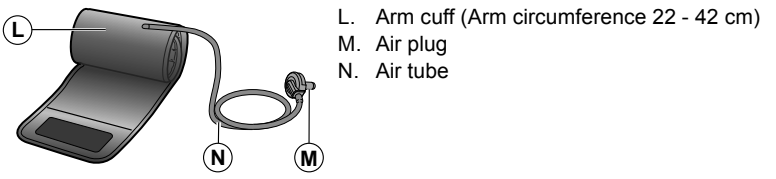

Display:

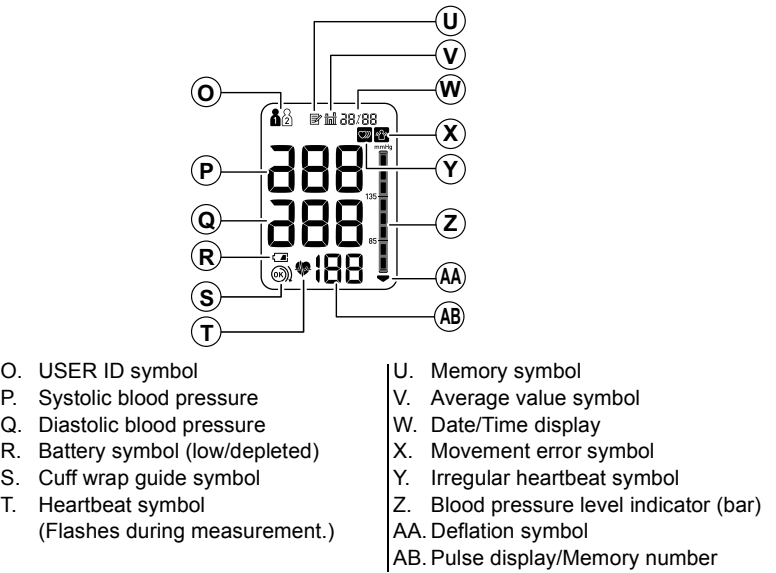


1.1 Display symbols:

**Irregular Heartbeat Symbol (Y)**

When the monitor detects an irregular rhythm two or more times during the measurement, the irregular heartbeat symbol will appear on the display with the measurement values.

An irregular heartbeat rhythm is defined as a rhythm that is 25% less or 25% more than the average rhythm detected while the monitor is measuring the systolic and diastolic blood pressure.

If the irregular heartbeat symbol displays with your measurement results, we recommend you consult your physician. Follow the directions of your physician.

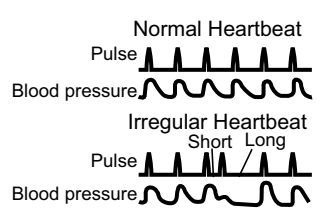

Movement Error Symbol (X)

The movement error symbol is displayed if you move your body during the measurement. Please remove the arm cuff, and wait 2 - 3 minutes. Take another measurement, remain still during measurement.

Average Value Symbol (V)

The average value symbol is displayed when you press and hold the memory button for more than 3 seconds. The most recent average value appears on the display screen.

Cuff Wrap Guide Lamp (F)

If the cuff was wrapped too loosely, it may cause unreliable values. If the wrapping of cuff is too loose, the cuff wrap guide lamp does not light. Otherwise F lights in green. This is the function which is used as an aid in determining if the cuff is wrapped snugly enough.

Blood Pressure Level Indicator (Colour)

If your systolic or diastolic pressure is above the standard range (135 mmHg for the systolic blood pressure and/or 85 mmHg for the diastolic blood pressure), the blood pressure level indicator (colour) will light in orange when the measurement result is displayed. If they are within the standard range, no light will appear.

The JNC7\* Guideline recommends the following guideline.

	General Guidelines for Blood Pressure	
	Prehypertension at Office	Hypertension at Home
Systolic Blood Pressure	120 - 139 mmHg	135 mmHg
Diastolic Blood Pressure	80 - 89 mmHg	85 mmHg

These are form statistical values for blood pressure.

\* JNC7: The Seventh Report, 2003 Dec, of the Joint National Committee on Prevention, Detection, Evaluation, and Treatment of High Blood Pressure.


1.2 Before Taking a Measurement

- To help ensure an accurate reading, follow these directions:
- Avoid bathing, drinking alcohol or caffeine, smoking, exercising and eating for 30 minutes before taking a measurement.
  - Rest for at least 5 minutes before taking the measurement.
  - Stress raises blood pressure. Avoid taking measurements during stressful times.
  - Measurements should be taken in a quiet place.
  - Remove tight-fitting clothing from your arm.

2. Preparation

2.1 Battery Installation

- Remove the battery cover.

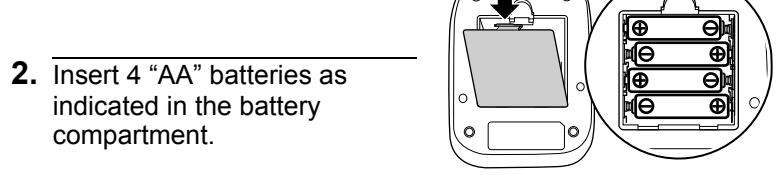

- Replace the battery cover.

- Notes:
- When the depleted battery symbol (E) appears on the display, turn the monitor off and remove all the batteries. Replace with 4 new batteries at the same time. Long life alkaline batteries are recommended.
  - The measurement values continue to be stored in memory even after the batteries are replaced.
  - The supplied batteries may have a shorter life.

Disposal of used batteries should be carried out in accordance with the national/local regulations for the disposal of batteries.

2.2 Setting the Date and Time

Set the monitor to the correct date and time before taking a measurement for the first time.

- Press the (C) button.
  - Push (Left) or (Right) to change the year.
- Push (C) button to confirm the year and then the month flashes. Repeat the same steps to change the month, day, hour, and minute.
- Year
- Month
- Day
- Hour
- Minute
- Change Confirm
- Forward : (Right)  
Back : (Left)

- Press the START/STOP button to turn the monitor off.


- Notes:
- If the batteries have been replaced, the date and time setting will need to be reset.
  - If the date and time are not set, "----" appears during or after measurement.

3. Using the Device

3.1 Applying the Arm Cuff


Remove tight-fitting clothing or tight rolled up sleeve from your left upper arm. Do not place the arm cuff over thick clothes.

- Insert the air plug into the air jack securely.
- Apply the arm cuff to your left upper arm.

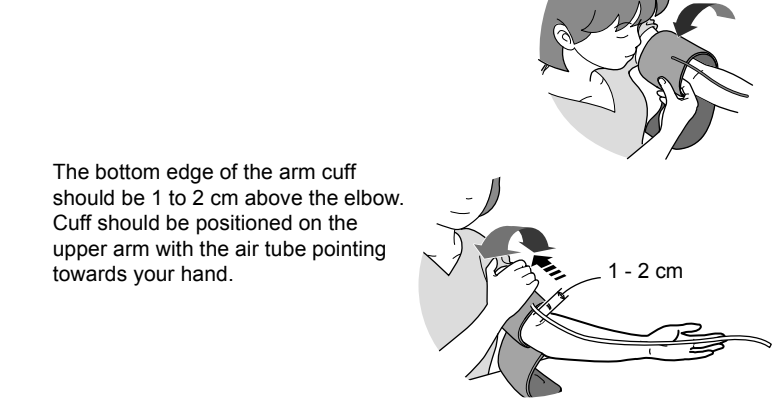

The bottom edge of the arm cuff should be 1 to 2 cm above the elbow. Cuff should be positioned on the upper arm with the air tube pointing towards your hand.

- Secure closed with the fabric fastener.

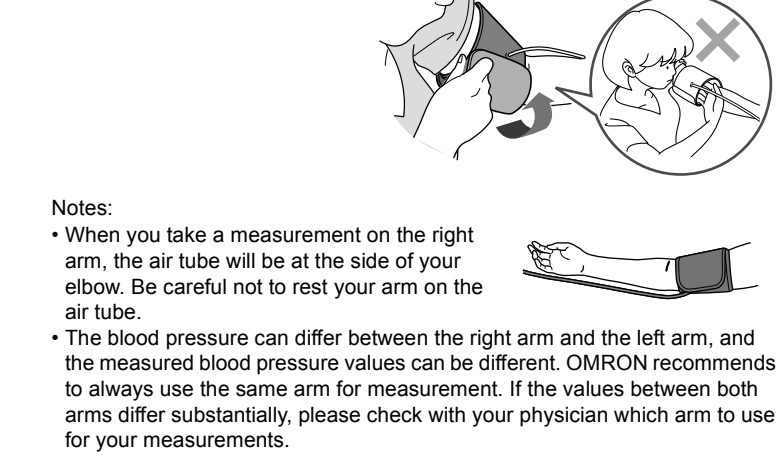


Notes:

- When you take a measurement on the right arm, the air tube will be at the side of your elbow. Be careful not to rest your arm on the air tube.
- The blood pressure can differ between the right arm and the left arm, and the measured blood pressure values can be different. OMRON recommends to always use the same arm for measurement. If the values between both arms differ substantially, please check with your physician which arm to use for your measurements.


3.2 How to Sit Correctly

To take a measurement, you need to be relaxed and comfortably seated, at a comfortable room temperature.

- Sit in a chair with your legs uncrossed and your feet flat on the floor.
- Sit with your back and arm being supported.
- The arm cuff should be placed on your arm at the same level as your heart.



The monitor is designed to take measurements and store the measurement values in the memory for 2 people using USER ID 1 and USER ID 2.

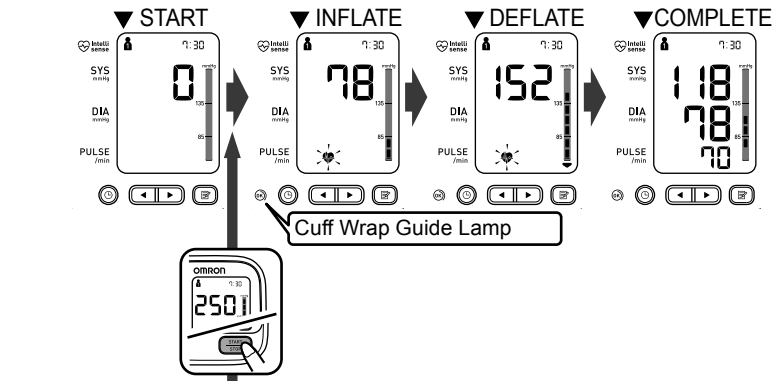- Select your USER ID (1 or 2).
  - Press the START/STOP button.
- The arm cuff will start to inflate automatically.
- 

Cuff Wrap Guide Lamp
- If your systolic pressure is more than 210 mmHg**

After the arm cuff starts to inflate, press and hold the START/STOP button until the monitor inflates 30 to 40 mmHg higher than your expected systolic pressure.

**Notes:**

  - The monitor will not inflate above 299 mmHg.
  - Do not apply more pressure than necessary.

- Remove the arm cuff.
- Press the START/STOP button to turn the monitor off.

The monitor automatically stores the measurement result in its memory. It will automatically turn off after 2 minutes.

Using the Guest Mode

The monitor stores measurement values for 2 users in the memory. The guest mode can be used to take a single measurement for another user. No measurement values are stored in the memory when the guest mode is selected.

- Press and hold the START/STOP button for more than 3 seconds. The USER ID symbol and the Date/Time display will disappear.
- Release the START/STOP button when the Date/Time display turns off.

The arm cuff will start to inflate automatically.

Always consult your physician. Self-diagnosis of measurement results and self-treatment are dangerous.


3.4 Using the Memory Function

The monitor automatically stores the results up to 60 sets for each user (1 and 2). It can also calculate an average value based on the last 3 measurement values taken within 10 minutes.

- Notes:
- If there are only 2 measurement values in the memory for that period, the average will be based on these 2 values.
  - If there is 1 measurement value in the memory for that period, this is displayed as the average.
  - If the memory is full, the monitor will delete the oldest value.
  - When viewing the measurement value taken without setting the date and time, "----" is displayed instead of the date and time.

To View the Measurement Values Stored in Memory


- Select your USER ID (1 or 2).
  - Press the (Memory) button.
- The Memory number appears for a second before the pulse rate is displayed. The newest set is numbered "1".

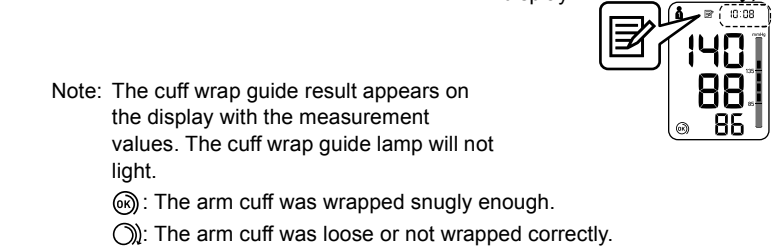

- Note: The cuff wrap guide result appears on the display with the measurement values. The cuff wrap guide lamp will not light.
- The arm cuff was wrapped snugly enough.
  - The arm cuff was loose or not wrapped correctly.
- Press the (Left) or (Right) button to view the values stored in memory.
- To view the older values
  - To view the more recent values

To View the Average Value

- Select your USER ID (1 or 2).
- Press and hold the (Memory) button for more than 3 seconds.

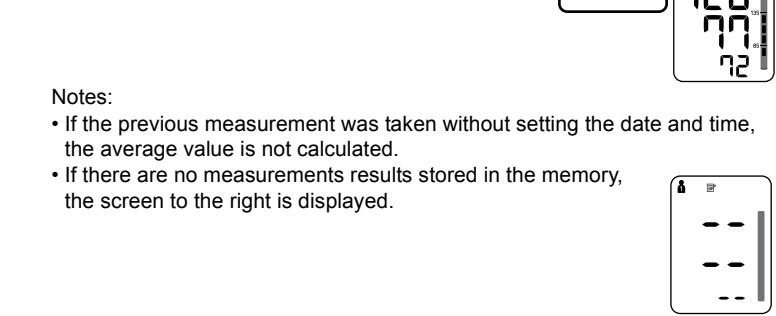


- Notes:
- If the previous measurement was taken without setting the date and time, the average value is not calculated.
  - If there are no measurements results stored in the memory, the screen to the right is displayed.

To Delete All the Values Stored in Memory

The values stored in the memory are deleted by USER ID.




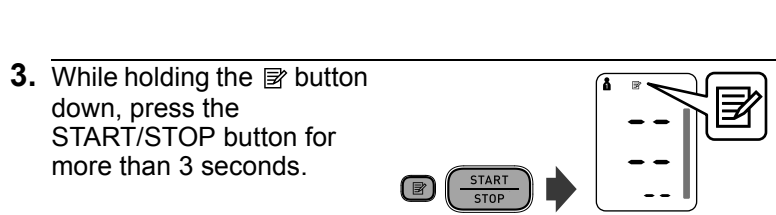








- Select your USER ID (1 or 2).
- Press the Memory button, while the memory symbol (Memory) appears.



Note: You cannot partially delete the values stored in the memory. All values for the user you select will be deleted.

4. Error Messages and Troubleshooting

4.1 Error Messages

Error Display	Cause	Solution
	Irregular heartbeats are detected.	Remove the arm cuff. Wait 2 - 3 minutes and then take another measurement. Repeat the steps in section3.3. If this error continues to appear, contact your physician.
	Movement during measurement.	Carefully read and repeat the steps in section 3.3.
	Arm cuff is applied too loosely.	Apply the arm cuff tighter. Refer to section 3.1.
	The batteries are low.	Recommend to replace the batteries with new ones ahead of time. Refer to section 2.1.
	The batteries are depleted.	Replace 4 batteries with new ones at once. Refer to section 2.1.
	Air plug disconnected.	Insert the plug securely. Refer to section 3.1.
	Arm cuff is applied too loosely.	Apply the arm cuff tighter. Refer to section 3.1.
	Air is leaking from the arm cuff.	Replace the cuff with a new one. Refer to section 5.3.
	Movement during measurement and the arm cuff has not been inflated sufficiently.	Repeat measurement. Remain still and do not talk during measurement. Refer to section 3.3.
		If "E2" appears repeatedly, inflate the cuff manually until it is 30 to 40 mmHg above your previous measurement result. Refer to section 3.3.
	The arm cuff was inflated exceeding the maximum allowable pressure, and then deflated automatically.	Do not touch the arm cuff and/or bend the air tube while taking a measurement. Do not inflate the arm cuff more than necessary. Refer to section 3.3.
	Movement during measurement.	Repeat measurement. Remain still and do not talk during measurement. Refer to section 3.3.
	Movement during measurement.	Repeat measurement. Remain still and do not talk during measurement. Refer to section 3.3.
	Clothing is interfering with the arm cuff.	Remove any clothing interfering with the arm cuff. Refer to section 3.1.
	Device error.	Contact your OMRON retail outlet or distributor.

4.2 Troubleshooting

In case of any of the below problems occur during measurement, first check that no other electrical device is within 30cm. If the problem persists, please refer to the table below.


Problem	Cause	Solution
The measurement result is extremely high (or low).	Arm cuff is applied too loosely.	Apply the arm cuff tighter. Refer to section 3.1.
	Movement or talking during measurement.	Remain still and do not talk during measurement. Refer to section 3.3.
Arm cuff pressure does not rise.	Clothing is interfering with the arm cuff.	Remove any clothing interfering with the arm cuff. Refer to section 3.1.
	The air connector is not securely connected into the air jack.	Make sure that the air tube is connected securely. Refer to section 3.1.
Arm cuff pressure does not rise.	Air is leaking from the arm cuff.	Replace the arm cuff with a new one. Refer to section 5.3.
	The arm cuff is loose.	Apply the cuff correctly so that it is firmly wrapped around the arm. Refer to section 3.1.
Cannot measure or the results are too low or too high.	The arm cuff has not been inflated sufficiently.	Inflate the cuff so that it is 30 to 40 mmHg above your previous measurement result. Refer to section 3.3.
Nothing happens when you press the buttons.	The batteries are depleted.	Replace 4 batteries with new ones. Refer to section 2.1.
	The batteries have been inserted incorrectly.	Insert the batteries with the correct (+/-) polarity. Refer to section 2.1.
Other problems.	• Press the START/STOP button and repeat measurement. • Replace the batteries with new ones. If the problem continues, contact your OMRON retail outlet or distributor.	

5. Maintenance and Storage

5.1 Maintenance

To protect your device from damage, please observe the following:

- Store the device and the components in a clean, safe location.
- Do not use any abrasive or volatile cleaners.
- Do not wash the device and any components or immerse them in water.
- Do not use petrol, thinners or similar solvents to clean the device.

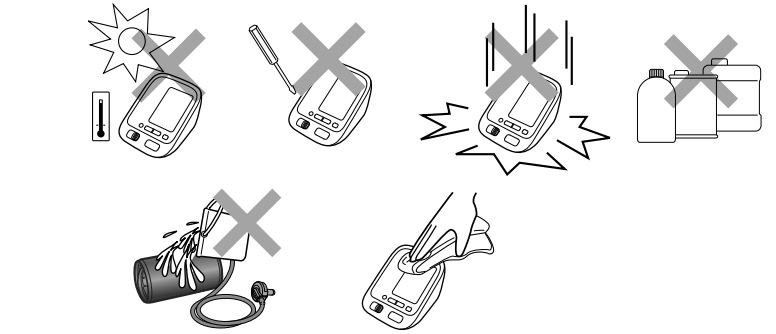

- Use a soft and dry cloth, or a soft and moistened cloth and neutral soap to clean on the monitor and the arm cuff.
- Changes or modification not approved by the manufacturer will void the user warranty. Do not disassemble or attempt to repair the device or components. Consult your authorised OMRON retail outlet or distributor.

Calibration and Service

- The accuracy of this blood pressure monitor has been carefully tested and is designed for a long service life.
- It is generally recommended to have the device inspected every 2 years to ensure correct functioning and accuracy. Please consult your authorised OMRON retail outlet or distributor.

5.2 Storage

Keep the device in its storage case when not in use.

1. Unplug the air plug from the air jack.
2. Gently fold the air tube into the arm cuff.


Note: Do not bend or crease the air tube excessively.

3. Place the monitor and the arm cuff in the storage case.

- Do not store the device in the following situations:
- If the device is wet.
  - Locations exposed to extreme temperatures, humidity, direct sunlight, dust or corrosive vapours such as bleach.
  - Locations exposed to vibrations, shocks or where it will be at an angle.

5.3 Optional Medical Accessories

(within the scope of EC Medical Device Directive 93/42/EEC)

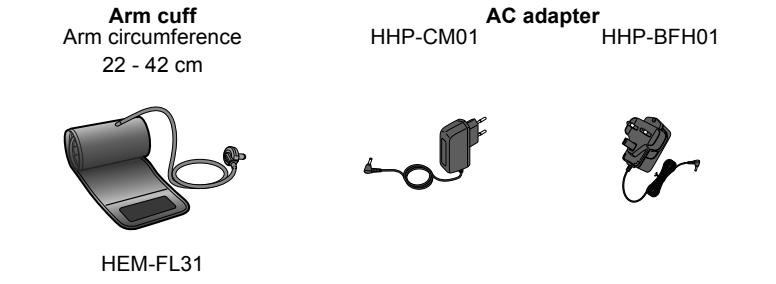

Using the Optional AC Adapter

Note: Make sure to use an easily accessible power socket in which to connect and disconnect the AC adapter.

1. Insert the AC adapter plug into the AC adapter jack on the rear side of the monitor.
2. Plug the AC adapter into an electrical outlet.

To disconnect the AC adapter, unplug the AC adapter from the electrical outlet first and then remove the AC adapter plug from the monitor.










6. Specifications




















<b>Product category</b>	Electronic Sphygmomanometers
<b>Product description</b>	Automatic Upper Arm Blood Pressure Monitor
<b>Model (code)</b>	M3 Comfort (HEM-7134-E)
<b>Display</b>	LCD Digital Display
<b>Measurement method</b>	Oscillometric method
<b>Measurement range</b>	Pressure: 0 to 299 mmHg Pulse: 40 to 180 beats/min.
<b>Blood pressure measurement range</b>	20 to 280 mmHg
<b>Pulse measurement range</b>	Pulse: 40 to 180 beats/min.
<b>Accuracy</b>	Pressure: ± 3 mmHg Pulse: ± 5% of display reading
<b>Inflation</b>	Fuzzy-logic controlled by electric pump
<b>Deflation</b>	Automatic pressure release valve
<b>Memory</b>	60 measurements with date and time for each user (1 and 2)
<b>Rating</b>	DC6V 4W
<b>Power source</b>	4 "AA" batteries 1.5V or optional AC adapter (INPUT AC100-240V 50/60Hz 0.12-0.065A)
<b>Durable period (Service life)</b>	Monitor: 5 years Cuff: 1 year Optional AC adapter: 5 years
<b>Battery life</b>	Approx. 1000 measurements (using new alkaline batteries)
<b>Applied part</b>	Type BF (Cuff)
<b>Protection against electric shock</b>	Internally powered ME equipment (When using only the batteries) Class II ME equipment (Optional AC adapter)
<b>IP classification</b>	Monitor: IP20 Optional AC adapter(HHP-CM01): IP21 Optional AC adapter(HHP-BFH01): IP22
<b>Operating conditions</b>	+10 to +40°C (50 to 104°F) 15 to 90% RH (non-condensing) 700 to 1060 hPa
<b>Storage/Transport conditions</b>	-20 to +60°C (-4 to 140°F) 10 to 95% RH (non-condensing) 700 to 1060 hPa
<b>Weight</b>	Monitor: Approx. 300 g without batteries Arm cuff: Approx. 163 g
<b>Outer dimensions</b>	Monitor: Approx. 107 (w) mm x 79 (h) mm x 141 (l) mm Arm cuff: Approx. 145 mm x 532 mm
<b>Cuff circumference</b>	22 to 42 cm
<b>Cuff / Tube material</b>	Nylon, polyester, polyvinyl chloride
<b>Package contents</b>	Monitor, arm cuff, instruction manual, storage case, battery set, blood pressure diary

- Notes:
- These specifications are subject to change without notice.
  - In the clinical validation study, the 5th phase was used on 85 subjects for determination of diastolic blood pressure.
  - This device is clinically investigated according to the requirements of ISO 81060-2:2013 (excluding pregnant and pre-eclampsia patients).
  - This device has been validated for use on pregnant and pre-eclampsia patients according to the Modified European Society of Hypertension Protocol\*
  - IP classification is degrees of protection provided by enclosures in accordance with IEC 60529.
  - The device and optional AC adapter are protected against solid foreign objects of 12.5 mm diameter and greater such as a finger. The optional AC adapter (HHP-CM01) is protected against vertically falling water drops which may cause issues during a normal operation. Another optional AC adapter (HHP-BFH01) is protected against oblique falling water drops which may cause issues during a normal operation.
  - This device can be used for continuous operation.
- \*Prof. Roland Asmar et al. publication pending

CE 0197

- This device fulfils the provisions of EC directive 93/42/EEC (Medical Device Directive).
- This blood pressure monitor is designed according to the European Standard EN1060, Non-invasive sphygmomanometers Part 1: General Requirements and Part 3: Supplementary requirements for electromechanical blood pressure measuring systems.
- This OMRON product is produced under the strict quality system of OMRON HEALTHCARE Co., Ltd., Japan. The Core component for OMRON blood pressure monitors, which is the Pressure Sensor, is produced in Japan.

Symbols description	
	Applied part - Type BF Degree of protection against electric shock (leakage current)
	Class II equipment. Protection against electric shock
<b>IP XX</b>	Ingress protection degree provided by IEC 60529
	CE Marking
	GOST-R symbol
	Metrology symbol
	Symbol of Eurasian Conformity
	Serial number
	LOT number
	Temperature limitation

	Humidity limitation
	Atmospheric pressure limitation
	Indication of connector polarity
	For indoor use only
	OMRON's trademarked technology for blood pressure measurement
	Identifier of cuffs compatible for the device
	Cuff positioning indicator for the left arm
	Artery Mark
	Range pointer and brachial artery alignment position
	Manufacturer's quality control mark
<b>LATEX FREE</b>	Not made with natural rubber latex
	Range indicator of arm circumferences to help selection of the correct cuff size.
	Need for the user to consult this instruction manual.
	Need for the user to follow this instruction manual thoroughly for your safety.
	Direct current
	Alternating current
	Date of manufacture
	Technology and Quality, JAPAN
	Technology and Design, JAPAN
	Arm circumference

Product production date is integrated in the Serial number, which is placed on the product and/or sales package: the first 4 digits mean year of production, the next 2 digits mean month of production.

**Important information regarding Electro Magnetic Compatibility (EMC)**  
HEM-7134-E manufactured by OMRON HEALTHCARE Co., Ltd. conforms to EN60601-1-2:2015 Electro Magnetic Compatibility (EMC) standard. Further documentation in accordance with this EMC standard is available at OMRON HEALTHCARE EUROPE at the address mentioned in this instruction manual or at [www.omron-healthcare.com](http://www.omron-healthcare.com). Refer to the EMC information for HEM-7134-E on the website.

Correct Disposal of This Product (Waste Electrical & Electronic Equipment)

This marking shown on the product or its literature, indicates that it should not be disposed of, with other household wastes at the end of its working life. To prevent possible harm to the environment or human health from uncontrolled waste disposal, please separate this product from other types of wastes and recycle it responsibly to promote the sustainable reuse of material resources.

Household users should contact either the retailer where they purchased this product, or their local government office, for details of where and how they can return this item for environmentally safe recycling.

Business users should contact their supplier and check the terms and conditions of the purchase contract. This product should not be mixed with other commercial waste for disposal.

7. Warranty

Thank you for buying an OMRON product. This product is constructed of high quality materials and great care has been taken in its manufacturing. It is designed to give you every satisfaction, provided that it is properly operated and maintained as described in the instruction manual.

This product is guaranteed by OMRON for a period of 3 years after the date of purchase. The proper construction, workmanship and materials of this product is guaranteed by OMRON. During this period of guarantee OMRON will, without charge for labour or parts, repair or replace the defect product or any defective parts.

The guarantee does not cover any of the following:

- a. Transport costs and risks of transport.
  - b. Costs for repairs and / or defects resulting from repairs done by unauthorised persons.
  - c. Periodic check-ups and maintenance.
  - d. Failure or wear of optional parts or other attachments other than the main device itself, unless explicitly guaranteed above.
  - e. Costs arising due to non-acceptance of a claim (those will be charged for).
  - f. Damages of any kind including personal caused accidentally or from misuse.
  - g. Calibration service is not included within the guarantee.
  - h. Optional parts have a one (1) year warranty from date of purchase. Optional parts include, but are not limited to the following items: Cuff and Cuff Tube, AC Adapter.
- Should guarantee service be required please apply to the dealer whom the product was purchased from or an authorised OMRON distributor. For the address refer to the product packaging / literature or to your specialised retailer.
- If you have difficulties in finding OMRON customer services, contact us for information.

[www.omron-healthcare.com](http://www.omron-healthcare.com)

Repair or replacement under the guarantee does not give rise to any extension or renewal of the guarantee period.

The guarantee will be granted only if the complete product is returned together with the original invoice / cash ticket issued to the consumer by the retailer.

8. Some Useful Information about Blood Pressure

What is Blood Pressure?


Blood pressure is a measure of the force of blood flowing against the walls of the arteries. Arterial blood pressure is constantly changing during the course of the heart's cycle. The highest pressure in the cycle is called the Systolic Blood Pressure; the lowest is the Diastolic Blood Pressure. Both pressures, the Systolic and Diastolic, are necessary to enable a physician to evaluate the status of a patient's blood pressure.

What is Arrhythmia?

Arrhythmia is a condition where the heartbeat rhythm is abnormal due to flaws in the bio-electrical system that drives the heartbeat. Typical symptoms are skipped heartbeats, premature contraction, an abnormally rapid (tachycardia) or slow (bradycardia) pulse.

Why is it a Good Thing to measure Blood Pressure at Home?

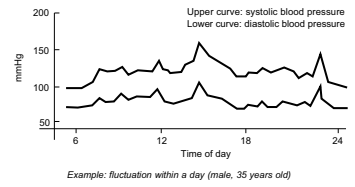

Many factors such as physical activity, anxiety, or the time of day, can influence your blood pressure. A single measurement may not be sufficient for an accurate diagnosis. Thus it is best to try and measure your blood pressure at the same time each day, to get an accurate indication of any changes in blood pressure. Blood pressure is typically low in the morning and increases from afternoon to evening. It is lower in the summer and higher in the winter.



How is Hypertension related to Stroke?

Hypertension (high blood pressure) is the key risk factor for Stroke. It is estimated that amongst hypertensive patients, effective treatment would prevent 1 in 4 haemorrhagic strokes (bleeding around the brain). Hypertension guidelines have endorsed the use of Home Blood Pressure Monitoring in addition to the measurements in physicians' offices to help manage hypertension effectively.

References to above medical claims are available upon request.

<b>Manufacturer</b> 	<b>OMRON HEALTHCARE Co., Ltd.</b> 53, Kunotsubo, Terado-cho, Muko, KYOTO, 617-0002 JAPAN
<b>EU-representative</b> 	<b>OMRON HEALTHCARE EUROPE B.V.</b> Scorpius 33, 2132 LR Hoofddorp, THE NETHERLANDS <a href="http://www.omron-healthcare.com">www.omron-healthcare.com</a>
<b>Production facility</b>	<b>OMRON HEALTHCARE MANUFACTURING VIETNAM CO., LTD.</b> No.28 VSIP II, Street 2, Vietnam-Singapore Industrial Park II, Binh Duong Industry-Services-Urban Complex, Hoa Phu Ward, Thu Dau Mot City, Binh Duong Province, Vietnam
<b>Subsidiaries</b>	<b>OMRON HEALTHCARE UK LTD.</b> Opal Drive, Fox Milne, Milton Keynes, MK15 0DG, UK <a href="http://www.omron-healthcare.com">www.omron-healthcare.com</a> <b>OMRON MEDIZINTECHNIK HANDELSGESELLSCHAFT mbH</b> Konrad-Zuse-Ring 28, 68163 Mannheim, GERMANY <a href="http://www.omron-healthcare.com">www.omron-healthcare.com</a> <b>OMRON SANTÉ FRANCE SAS</b> 14, rue de Lisbonne, 93561 Rosny-sous-Bois Cedex, FRANCE <a href="http://www.omron-healthcare.com">www.omron-healthcare.com</a>

Made in Vietnam